

Table 1: Date and Quantity of Applied Copper-based Crop Protectant in Relation to Simulated Rain Event Dates.

Date	Crop Protectant Applied to Each Plasticulture Tomato Field			Simulated Rain Event Number
	Application Number	Volume, L	Cu Mass per Field, g	
29-Jun	1	0.50	1	---
6-Jul	2	0.50	1.52	---
19-Jul	3	0.50	0.85	---
31-Jul	---	---	---	1
5-Aug	4	0.63	1.13	---
6-Aug	---	---	---	2
12-Aug	5	0.50	1.04	---
17-Aug	6	0.33	0.81	---
18-Aug	---	---	---	3
25-Aug	7	0.33	0.6	---
2-Sep	---	---	---	4
7-Sep	8	0.50	1.09	---
9-Sep	---	---	---	5
18-Sep	9	0.33	0.69	6
24-Sep	10	0.33	0.57	---
25-Sep	---	---	---	7
1-Oct	11	0.33	0.63	---
2-Oct	---	---	---	8
21-Oct	---	---	---	9

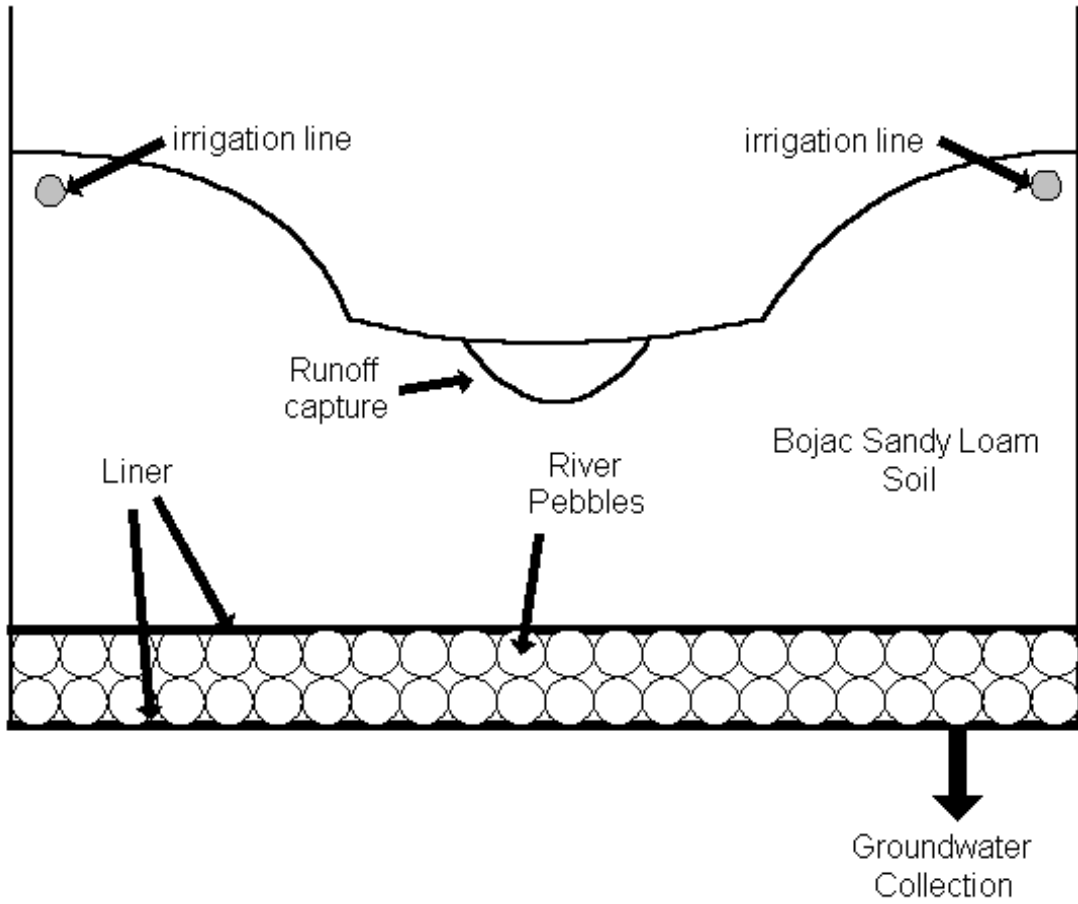


Figure 1: Cross-sectional Drawing of Simulated Tomato Field.